

LOCTITE®



LOCTITE® 3D MED3394™

Sterilizable
Sheer Black, White

LOCTITE®

Henkel Corporation

loctite3dp@henkel.com





MED3394™
STERILIZABLE



LOCTITE 3D MED3394™

LOCTITE 3D MED3394 is a high-performance material developed to withstand the harsh environment created during sterilization cycles. The high temperature resistance and low water absorption means it can withstand multiple autoclave cycles.

LOCTITE 3D MED3394 is capable of meeting ISO 10993-5, -10, -11 (acute systemic) and -23 standards, as well as USP Class VI, for biocompatibility when processed using a validated workflow. Certificates of Compliance are available upon request.

LOCTITE 3D MED3394 exhibits is available in both white and sheer black colors and can print on a variety of DLP, LCD, and mSLA style resin 3D printers.



Benefits:

- High heat resistance, HDT 100°C
- Excellent biocompatibility
- Low water absorption



Ideal for:


- Medical Devices
- Laboratory Equipment
- Sterile Devices
- Cleanroom environments



Markets:



Healthcare

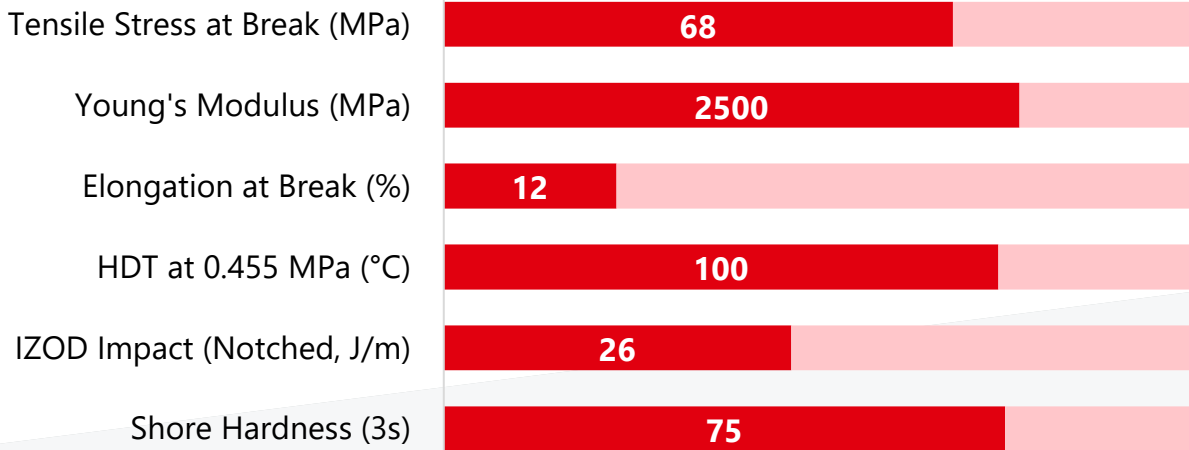



MED3394™
STERILIZABLE
SHEER BLACK



PROPERTIES

Mechanical Properties	Measure	Method	Green	Post Processed
Young's Modulus	MPa	ASTM D638	1400 - 1700 ^[1]	2450 - 2650 ^[1]
Tensile Stress at Yield	MPa	ASTM D638	34 - 44 ^[1]	68 - 76 ^[1]
Elongation at Yield	%	ASTM D638	3.9 - 4.4 ^[1]	4.5 - 4.9 ^[1]
Tensile Stress at Break	MPa	ASTM D638	31 - 38 ^[1]	66 - 72 ^[1]
Elongation at Break	%	ASTM D638	25 - 39 ^[1]	9 - 16 ^[1]
Flexural Modulus	MPa	ASTM D790	-	2450 - 2750 ^[1]
Flexural Stress at Break	MPa	ASTM D790	-	-
Flexural Elongation at Break	%	ASTM D790	>5 ^[1]	>5 ^[1]
IZOD Impact (Notched)	J/m	ASTM D256	-	24.5 - 27.5 ^[1]
Shore Hardness (3s)	D	ASTM D2240	66 ^[2]	75 ^[2]
Other Properties				
HDT at 0.455 MPa	°C	ASTM D648	-	97 - 104 ^[1]
HDT at 1.82 MPa	°C	ASTM D648	-	82 - 94 ^[1]
Water Absorption (24hr)	%	ASTM D570	-	0.53 ^[3]
Water Absorption (48hr)	%	ASTM D570	-	0.69 ^[3]
Water Absorption (72hr)	%	ASTM D570	-	0.90 ^[3]
Solid Density	g/cm ³	ASTM D792	1.14 ^[4]	1.15 ^[4]
CTE (10°C to 60°C)	µm/(m·K)	ASTM E831	-	92.3 ^[5]

Test parameters:

"All specimen are printed unless otherwise noted. All specimen were conditioned in ambient lab conditions at 19-23°C / 40-60% RH for at least 24 hours." ASTM Methods: D638 Type IV, 5 mm/min, D790-B, 13 mm/min, D648, D256 Notched IZOD (Machine Notched), 6 mm x 12 mm, D570 0.125" x 2" Disc 24hr@ 25°C, D2240, Type "D" (3 seconds), D7867, D1475

Internal Data Sources:

[1] GEN676679, [2] FOR600710, [3] FOR610015, [4] FOR554095, [5] FOR670854





MED3394™
STERILIZABLE
SHEER BLACK



PROPERTIES

Biocompatibility	Method	Green	Post Processed
Cytotoxicity	ISO 10993-5	-	Comply ^[1]
Sensitization	ISO 10993-10	-	Comply ^[2]
Acute Systemic Toxicity	ISO 10993-11	-	Comply ^[3]
Irritation	ISO 10993-23	-	Comply ^[4]
USP Class VI	-	-	Comply ^[5]
Sterility via Autoclave	Internal	-	Comply ^[10]

Liquid Properties	Measure	Method	Value
Viscosity at 25°C (77°F)	cP	ASTM D7867	1100 - 1250 ^[6]
Liquid Density	g/cm ³	ASTM D1475	1.09 ^[7]

Electrical Properties	Measure	Method	Green	Post Processed
Volume Resistivity	Ω·cm	ASTM D257	-	1.05E + 16 ^[8]
Surface Resistivity	Ω	ASTM D257	-	4.0E + 11 ^[9]
AC Relative Permittivity (Dielectric Constant) ^[8]				
at 50 Hz (XY)	none	ASTM D150	-	3.8
at 1 kHz (XY)	none	ASTM D150	-	3.7
at 1 MHz (XY)	none	ASTM D150	-	3.4
AC Loss Characteristic (Dissipation Factor) ^[8]				
at 50 Hz (XY)	none	ASTM D150	-	0.010
at 1 kHz (XY)	none	ASTM D150	-	0.010
at 1 MHz (XY)	none	ASTM D150	-	0.027

Test parameters:

All specimen are printed unless otherwise noted. All specimen were conditioned in ambient lab conditions at 19-23°C / 40-60% RH for at least 24 hours. ASTM Methods: D7867, D1475

Internal Data Sources:

[1] FOR653183, [2] FOR653182, [3] FOR653184, [4] FO653181, [5] FOR660013, [6] FO674935, [7] FOR554095, [8] FOR665372, [9] FOR684560, [10] FOR679644





WORKFLOW

Validated workflows need to be followed to achieve properties as provided in the TDS. Examples of validated workflow steps are listed below. Users should defer to the most current workflow information for best results which can be found at <https://www.loctiteam.com/printer-validation-settings>

PRINTER SETTINGS

LOCTITE 3D MED3394 SHR BK is formulated to print optimally on an industrial DLP printer. Read the safety data sheet carefully to get details about health and safety instructions. Recommended print parameters:

- Shake resin bottle well before usage
- Temperature: 20°C to 35°C
- Intensity: 3 mW/cm² to 7 mW/cm²

Settings: 385 nm at 5 mW/cm ²	Measure	Method	Value
Layer Thickness	µm	Internal	100
Burn-in Region	s	Internal	40
Transition Region	s	Internal	15
Model Region	s	Internal	4.5

Settings: 385 nm at 5 mW/cm ²	Measure	Method	Value
E _C	mJ/cm ²	Internal	10.6 ^[1]
D _P	mm	Internal	0.32 ^[1]

Settings: 385 nm at 5 mW/cm ²	Measure	Method	Exposure time
D _C = 50 µm	s	Internal	2.5*
D _C = 100 µm	s	Internal	2.9*

Test parameters:

*Exposure times are calculated without a safety factor

Internal data source:

[1] FOR602556





WORKFLOW

Validated workflows need to be followed to achieve properties as provided in the TDS. Examples of validated workflow steps are listed below. Users should defer to the most current workflow information for best results which can be found at <https://www.loctiteam.com/printer-validation-settings>

CLEANING

LOCTITE 3D MED3394 SHR BK requires post processing to achieve specified properties. Prior to post curing, support structures should be removed from the printed part, and the part should then be washed. Use compressed air to remove residual solvent from the surface of the material between intervals.

Post Process Step	Agent	Method	Duration	Intervals	Additional Info
Cleaning Step #1	IPA	Ultrasonic	2 min	2	Dry after each interval
Dry	n.a.	Compressed air	10 s to 60 s	1	Air pressure (50psi)
Wait before post curing	n.a.	Ambient condition	60 min	1	Room temperature

POST CURING

LOCTITE 3D MED3394 SHR BK requires post curing to achieve specified properties. It is recommended that either an LED or wide spectrum lamp be used to post cure parts.

An additional heat cure at 100°C for one hour is recommended for most workflows to realize highest HDT performance. Allow the parts to rest one hour between UV cure and heat cure. To minimize risk of warpage place parts in cold oven before ramping up temperature to target value and cool down parts slowly in switched off oven after reaching the heat curing conditions.

UV Curing Unit	UV Source	Intensity	Cure time per side	Additional Settings (Shelf, Output Energy)
Dymax 5000 EC Flood	Mercury Arc Bulb (broad spectrum)	150 mW/cm ² at 380 nm	10 min	400W, Shelf K
Loctite CL36	405nm LED	80 mW/cm ² at 405 nm	10 min	100% top & side



LOCTITE®

MED3394™
STERILIZABLE
SHEER BLACK



WORKFLOW

Validated workflows need to be followed to achieve properties as provided in the TDS. Examples of validated workflow steps are listed below. Users should defer to the most current workflow information for best results which can be found at <https://www.loctiteam.com/printer-validation-settings>

STORAGE

Store **LOCTITE 3D MED3394 SHR BK** in the unopened container in a dry location. Optimal Storage: 8°C to 30°C. Storage below 8°C or above 30°C can adversely affect product properties. Material removed from containers may be contaminated during use. For this reason, filter used resin with 190 µm mesh filter before placing back into proper storage container.









MED3394™ STERILIZABLE SHEER BLACK



AGEING AND ENVIRONMENTAL EFFECTS – STERILIZATION

LOCTITE 3D MED3394 SHR BK was sterilized via a variety of sterilization methods. Sterilized samples were conditioned for a minimum of 24 hours before mechanical testing. Control samples were stored at a constant 22°C. All samples were printed using a validated workflow. Mechanical testing was conducted according to ASTM D638 at standard lab conditions (22°C).

Data represents mechanical properties shortly after sterilization and are not indicative of long-term shelf-aged performance.

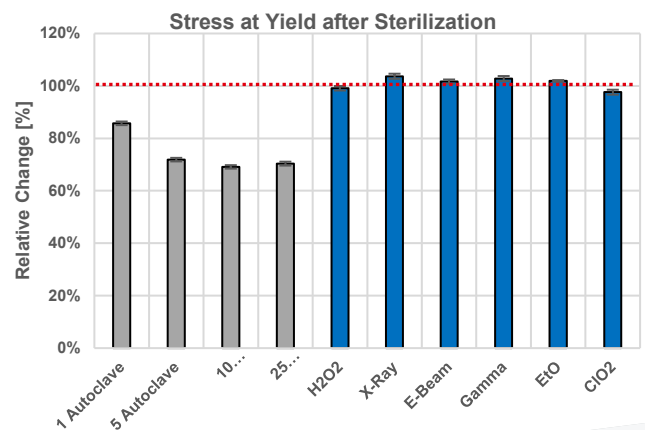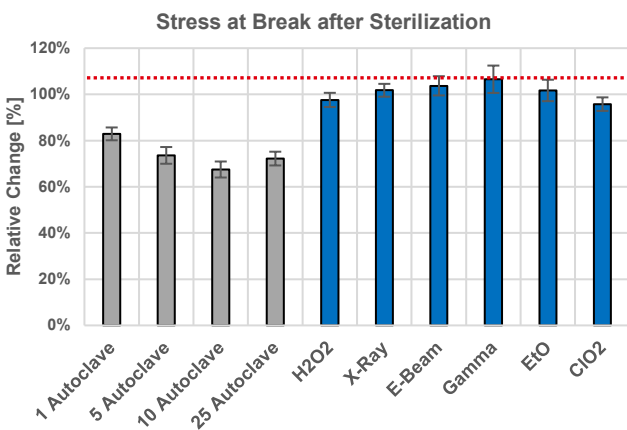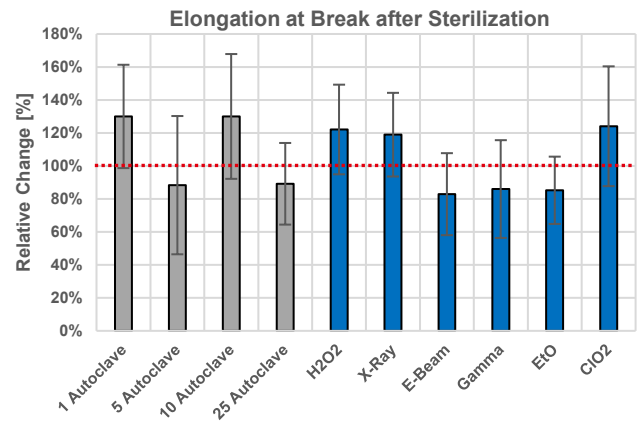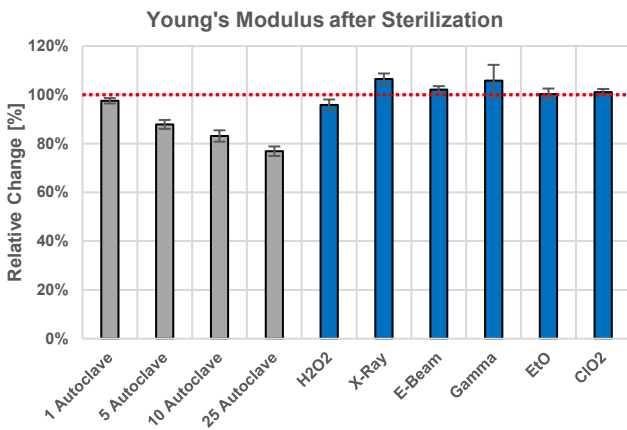

Test parameters:

ASTM D638: Type IV, Pull speed: 5 mm/min, Young's modulus measured at 0.1-1.0% (regression), 22°C. Sterilization Information: Autoclave – 134°C for 18 minutes at 2.1 bar, H2O2 – 4 injection sterilization cycle of 59% H2O2, X-Ray – 11kGy nominal dose, E-Beam – 11kGy nominal dose, Gamma – 40kGy nominal dose, EtO – 3 cycles, ClO2 – under vacuum conditions.

Internal Data Sources:
[GEN685128](#)









AGEING AND ENVIRONMENTAL EFFECTS – HEAT AGEING

LOCTITE 3D MED3394 SHR BK was heat aged without load according to ASTM D3045. Test samples were exposed for a defined time at 50°C and conditioned for 24 hours at 22°C before mechanical testing. Control samples were stored at a constant 22°C. All samples were printed in the same print job using a validated workflow. Mechanical testing was conducted according to ASTM D638 at standard lab conditions (22°C).

“0 weeks” represents non-aged samples stored at 22°C and tested 24 hours after post-processing.

Based on temperature dependence of reaction rates a test time of 6 weeks at 50°C can be interpreted as approximately 12 months at ambient temperature.

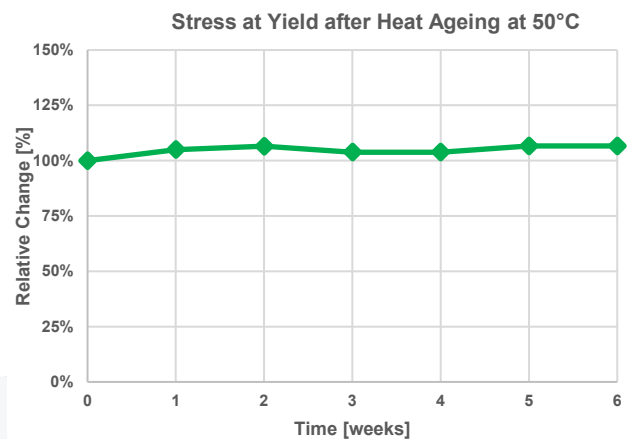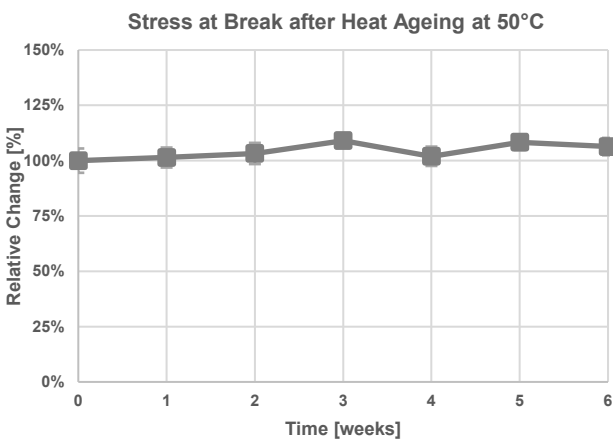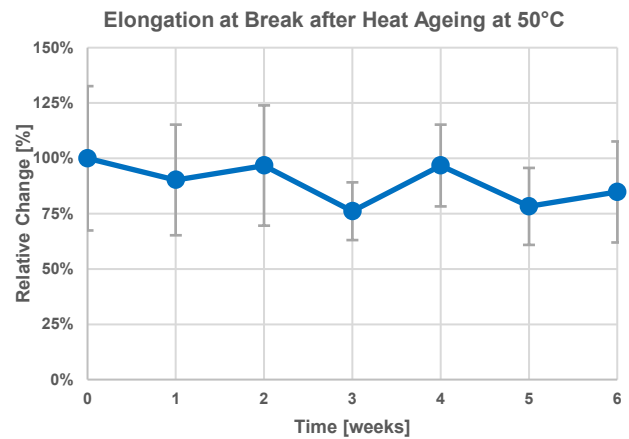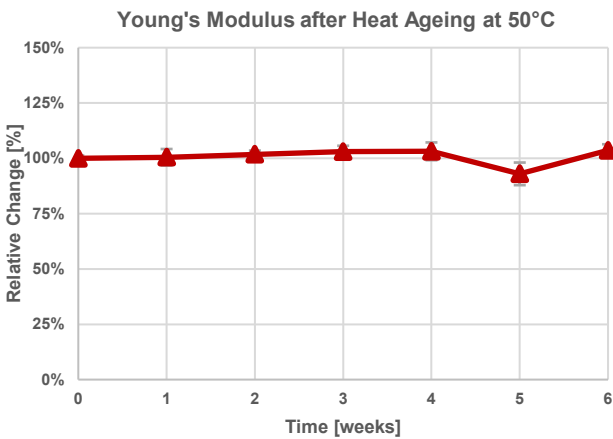

Test parameters:
ASTM D638: Type IV, Pull speed: 5 mm/min, Young's modulus measured at 0.1-1.0% (regression), 22°C

Internal Data Sources:
[FOR635905](#), [FOR635909](#)









MED3394™
STERILIZABLE
SHEER BLACK



AGEING AND ENVIRONMENTAL EFFECTS – ACCELERATED WEATHERING (UV AGEING)

LOCTITE 3D MED3394 SHR BK has been tested after accelerated outdoor weathering according to ASTM D4329 (Cycle A). Test samples were exposed to defined conditions of heat, water condensation and UV light. Exposed samples were conditioned for 24 hours at 22°C before mechanical testing. Control samples were stored at a constant 22°C. All samples were printed in the same print job using a validated workflow. Mechanical testing was conducted according to ASTM D638 at standard lab conditions (22°C). "0 weeks" represents non-aged samples stored at 22°C and tested 24 hours after post-processing.

Please note, accelerated weathering testing can never fully represent real outdoor conditions and complexity. It is therefore recommended to conduct additional (outdoor) testing relevant for your specific application needs.

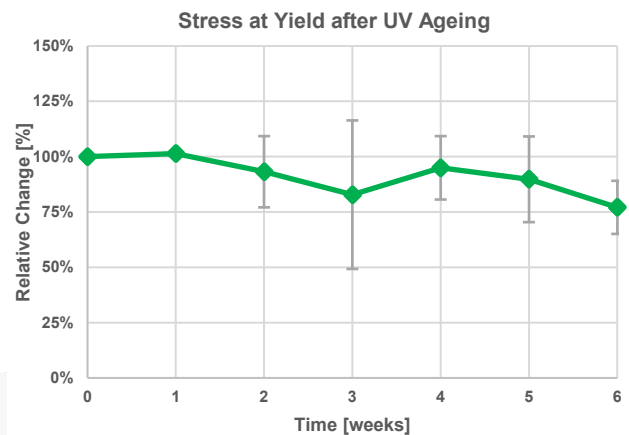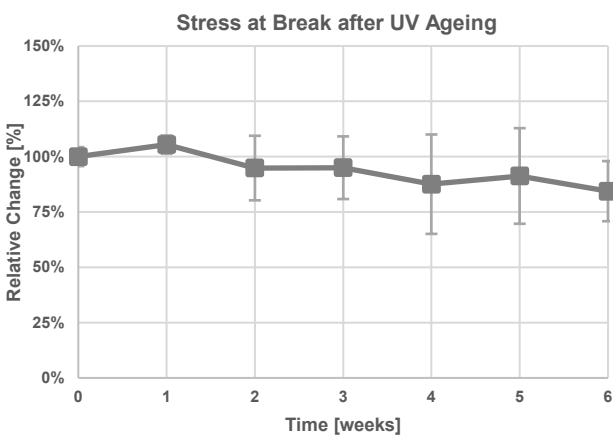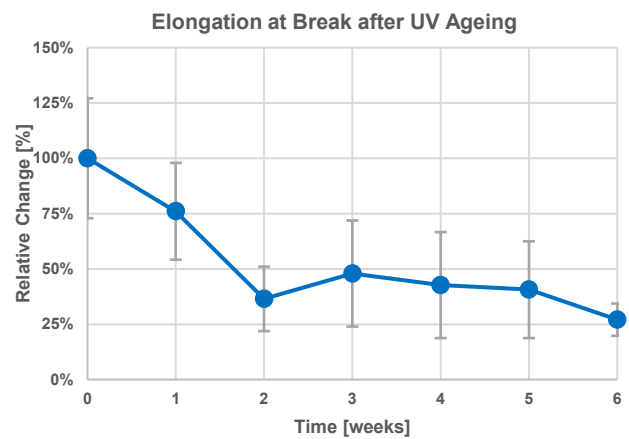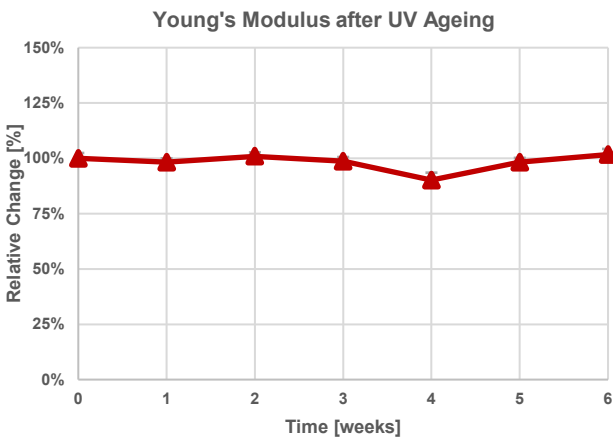

Test parameters:
ASTM D638: Type IV, Pull speed: 5 mm/min, Young's modulus measured at 0.1-1% (regression), 22 °C
ASTM D4329: Cycle A for general applications, QUV/se, UVA 340 nm, 0.89 W/m²·nm, 8 hours UV light at 60°C followed by 4 hours at 50°C condensation in the dark. To reduce any sample warpage during test time samples were placed in tailor-made holders without any fixation clamps or mechanical load. Exposed samples were always removed from QUV before next condensation cycle to avoid samples that are soaked excessively with water before testing.

Internal Data Sources:
[FOR640990](#), [FOR640994](#)







THERMAL INFLUENCE ON MECHANICAL PROPERTIES

LOCTITE 3D MED3394 SHR BK has been tested according to ASTM D638 at varied environmental temperatures, from -40°C to 100°C. All samples were printed in the same print job using a validated workflow. Mechanical testing was conducted according to ASTM D638. Before each test series samples were conditioned for 60 minutes at the specific test temperature.


Young's Modulus at -40°C to 100 °C

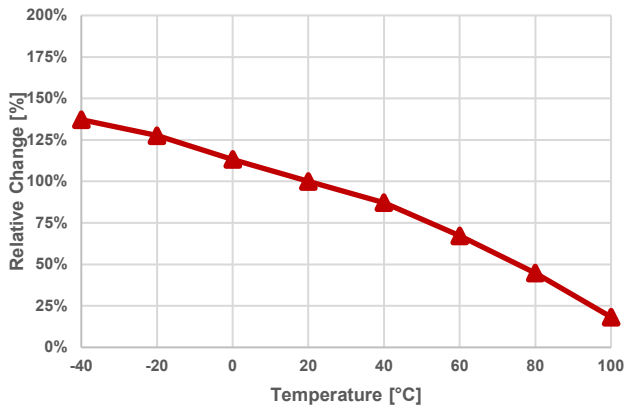


Elongation at Break at -40°C to 100 °C

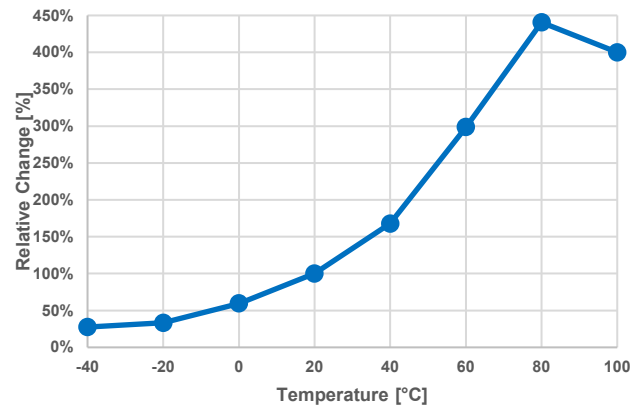

Stress at Break at -40°C to 100 °C

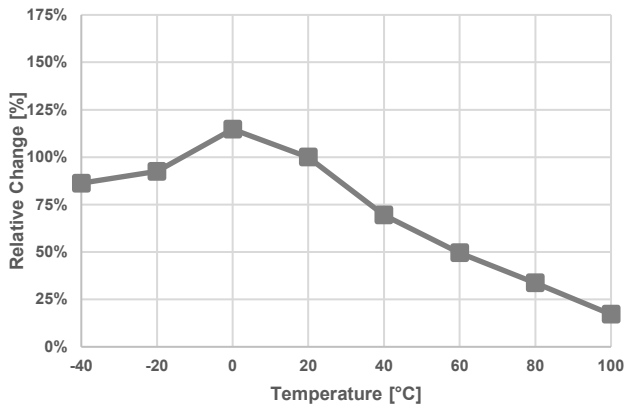

Stress at Yield at -40°C to 100 °C

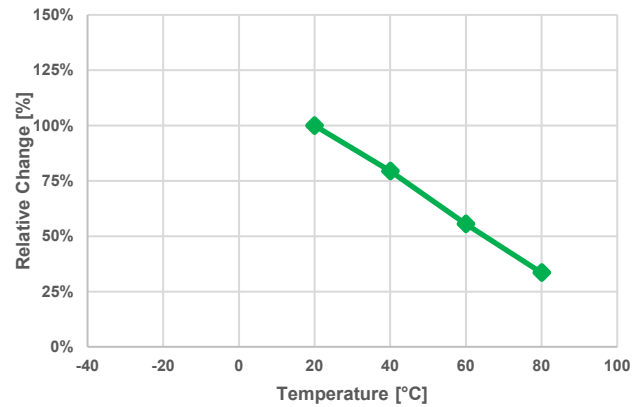

Test parameters:
ASTM D638, Type IV, Pull speed: 5 mm/min, Young's modulus measured at 0.1-1% (regression)

Internal Data Sources:
[FOR667304](#), [FOR669197](#)









AGEING AND ENVIRONMENTAL EFFECTS – CHEMICAL RESISTANCE MEDICAL

LOCTITE 3D MED3394 SHR BK has been tested after chemical ageing according to ASTM D543. The influence of chemicals was tested by measuring mechanical properties after different test times (Immersion test for 24 and 168 hours). Exposed samples were stored in containers and fully immersed in different chemicals. Samples were stirred every 24 hours using a shaker. After removal, exposed samples were washed and conditioned for 24 hours at 22°C before mechanical testing. All samples were printed using a validated workflow. Mechanical testing was conducted according to ASTM D638 at standard lab conditions (22°C).

“100%” represents non-aged samples stored at 22°C and tested 24 hours after post-processing.

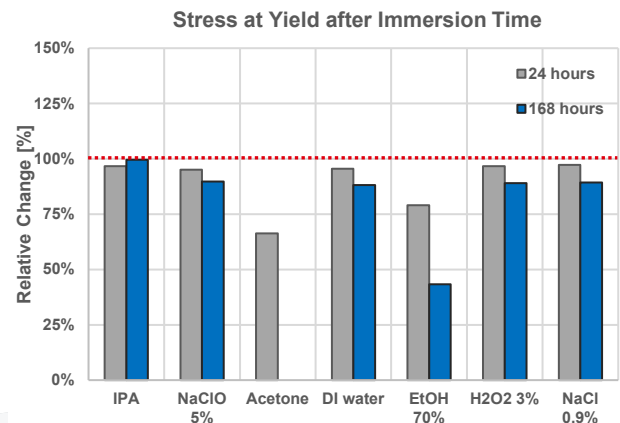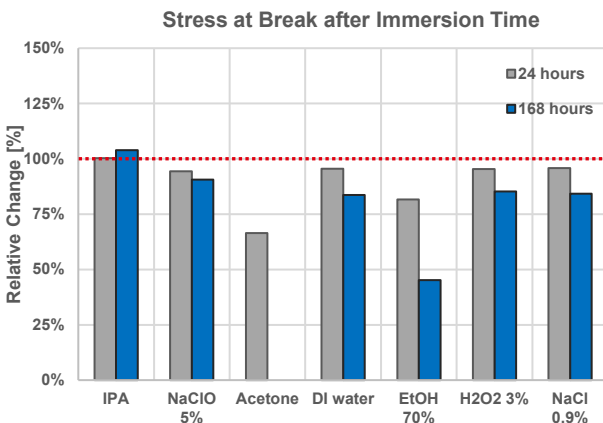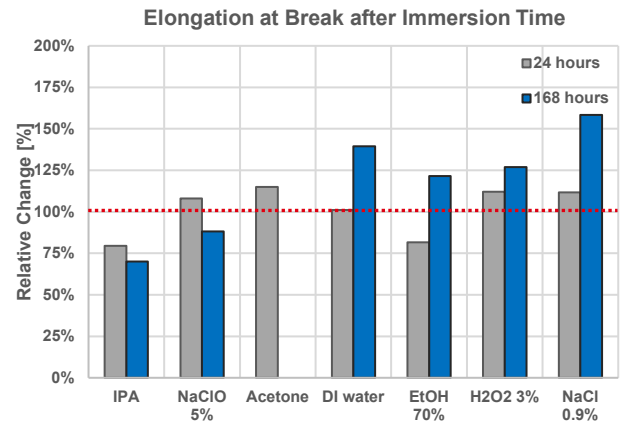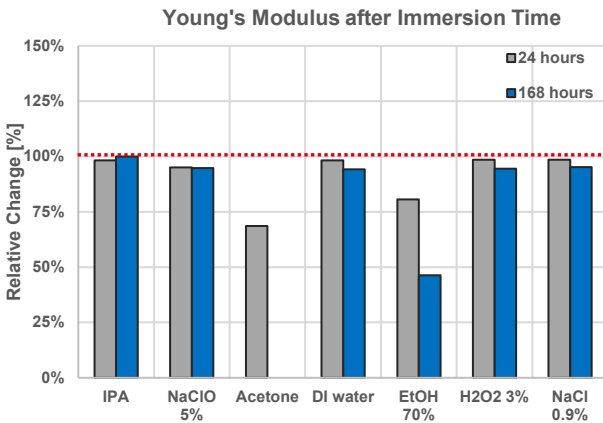

Test parameters:
ASTM D638: Type IV, Pull speed: 5 mm/min, Young's modulus measured at 0.1-1.0% (regression), 22°C
ASTM D543: Samples immersed in different chemicals were stored at 22°C.

Internal Data Sources:
FOR669958, FOR669957, FOR669960, FOR676378, FOR669962, FOR676381, FOR676383






MED3394™
STERILIZABLE
SHEER BLACK



AGEING AND ENVIRONMENTAL EFFECTS – CHEMICAL RESISTANCE MASS SOAK

LOCTITE 3D MED3394 SHR BK has been tested after chemical ageing according to ASTM D543. The influence of chemicals was tested by measuring the mass change after different test times (Immersion test for 24 and 168 hours). Exposed samples were stored in containers and fully immersed in different chemicals. Samples were stirred every 24 hours using a shaker. After removal exposed samples were washed, dried and immediately weighed. All samples were printed using a validated workflow.

“100%” represents the initial weight 24 hours after post-processing.

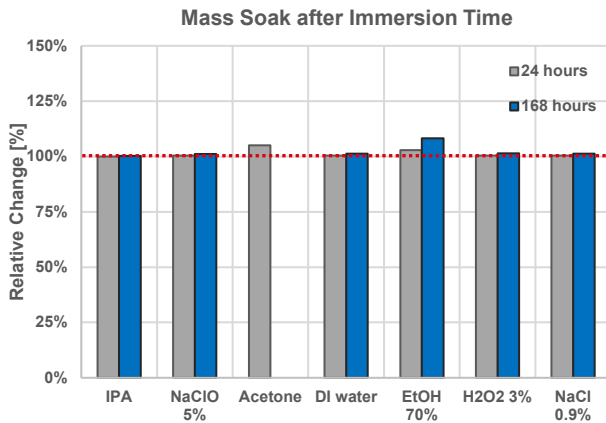

Test parameters:
ASTM D543: Samples immersed in different chemicals were stored at 22°C.


Internal Data Sources:
[FOR669958](#), [FOR669957](#), [FOR669960](#), [FOR676378](#), [FOR669962](#), [FOR676381](#), [FOR676383](#)





MED3394™

STERILIZABLE
WHITE

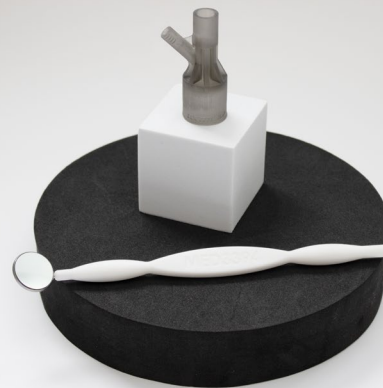

PROPERTIES

Mechanical Properties	Measure	Method	Green	Post Processed
Young's Modulus	MPa	ASTM D638	1400 - 1850 ^[1]	2400 - 2750 ^[1]
Tensile Stress at Yield	MPa	ASTM D638	35 - 46 ^[1]	67 - 72 ^[1]
Elongation at Yield	%	ASTM D638	3.9 - 4.2 ^[1]	4.4 - 4.7 ^[1]
Tensile Stress at Break	MPa	ASTM D638	31 - 36 ^[1]	64 - 70 ^[1]
Elongation at Break	%	ASTM D638	18 - 33 ^[1]	9 - 13 ^[1]
Flexural Modulus	MPa	ASTM D790	-	2300 ^[1]
Flexural Stress at Break	MPa	ASTM D790	-	-
Flexural Elongation at Break	%	ASTM D790	>5 ^[2]	>5 ^[2]
IZOD Impact (Notched)	J/m	ASTM D256	-	26.5 - 27.5 ^[1]
Shore Hardness (3s)	D	ASTM D2240	-	74 ^[2]
Other Properties				
HDT at 0.455 MPa	°C	ASTM D648	-	97 - 100 ^[1]
HDT at 1.82 MPa	°C	ASTM D648	-	80 - 84 ^[1]
Water Absorption (24hr)	%	ASTM D570	-	0.73 ^[2]
Water Absorption (48hr)	%	ASTM D570	-	0.85 ^[2]
Water Absorption (72hr)	%	ASTM D570	-	0.86 ^[2]
Solid Density	g/cm ³	ASTM D792	1.15 ^[2]	1.20 ^[2]
CTE (10°C to 60°C)	µm/(m·K)	ASTM E831	-	91.3 ^[6]

Test parameters:

"All specimen are printed unless otherwise noted. All specimen were conditioned in ambient lab conditions at 19-23°C / 40-60% RH for at least 24 hours." ASTM Methods: D638 Type IV, 5 mm/min, D790-B, 1.3 mm/min, D648, D256 Notched IZOD (Machine Notched), 6 mm x 12 mm, D570 0.125" x 2" Disc 24hr@ 25°C, D2240, Type "D" (3 seconds), D7867, D1475

Internal Data Sources:

[1] GEN685172, [2] FOR623072, [3] FOR610015, [4] FOR554095, [5] FOR644291, [6] FOR670853





PROPERTIES

Biocompatibility	Method	Green	Post processed
Cytotoxicity	ISO 10993-5	-	Comply ^[1]
Sensitization	ISO 10993-10	-	Comply ^[2]
Acute Systemic Toxicity	ISO 10993-11	-	Comply ^[2]
Irritation	ISO 10993-23	-	Comply ^[2]
USP Class VI	-	-	Comply ^[2]
Sterility via Autoclave	Internal	-	Comply ^[6]

Liquid Properties	Measure	Method	Value
Viscosity at 25°C (77°F)	cP	ASTM D7867	1150 - 1300 ^[3]
Liquid Density	g/cm ³	ASTM D1475	1.09 ^[4]

Electrical Properties	Measure	Method	Green	Post Processed
Volume Resistivity	Ω·cm	ASTM D257	-	8.49E + 15 ^[5]
AC Relative Permittivity (Dielectric Constant) ^[5]				
at 50 Hz (XY)	none	ASTM D150	-	3.9
at 1 kHz (XY)	none	ASTM D150	-	3.8
at 1 MHz (XY)	none	ASTM D150	-	3.5
AC Loss Characteristic (Dissipation Factor) ^[5]				
at 50 Hz (XY)	none	ASTM D150	-	0.009
at 1 kHz (XY)	none	ASTM D150	-	0.010
at 1 MHz (XY)	none	ASTM D150	-	0.031

Test parameters:

All specimen are printed unless otherwise noted. All specimen were conditioned in ambient lab conditions at 19-23°C / 40-60% RH for at least 24 hours. ASTM Methods: D7867, D1475

Internal Data Sources:

[1] FOR6667411, [2] GEN747261, [3] FOR674931, [4] FOR623072, [5] FOR671965, [6] FOR679644





WORKFLOW

Validated workflows need to be followed to achieve properties as provided in the TDS. Examples of validated workflow steps are listed below. Users should defer to the most current workflow information for best results which can be found at <https://www.loctiteam.com/printer-validation-settings>

PRINTER SETTINGS

LOCTITE 3D MED3394 WH is formulated to print optimally on an industrial DLP printer. Read the safety data sheet carefully to get details about health and safety instructions. Recommended print parameters:

- Shake resin bottle well before usage
- Temperature: 20°C to 35°C
- Intensity: 3 mW/cm² to 7 mW/cm²

Settings: 385 nm at 5 mW/cm ²	Measure	Method	Value
Layer Thickness	µm	Internal	100
Burn-in Region	s	Internal	20
Transition Region	s	Internal	12
Model Region	s	Internal	6

Settings: 385 nm at 5 mW/cm ²	Measure	Method	Value
E _C	mJ/cm ²	Internal	6.0 ^[1]
D _p	mm	Internal	0.14 ^[1]

Settings: 385 nm at 5 mW/cm ²	Measure	Method	Exposure time
D _C = 50 µm	s	Internal	1.7*
D _C = 100 µm	s	Internal	2.5*

Test parameters:
Exposure times are calculated without a safety factor

Internal data source:
[9] FOR623088





MED3394™
STERILIZABLE
WHITE



WORKFLOW

Validated workflows need to be followed to achieve properties as provided in the TDS. Examples of validated workflow steps are listed below. Users should defer to the most current workflow information for best results which can be found at <https://www.loctiteam.com/printer-validation-settings>

CLEANING

LOCTITE 3D MED3394 WH requires post processing to achieve specified properties. Prior to post curing, support structures should be removed from the printed part, and the part should then be washed. Use compressed air to remove residual solvent from the surface of the material between intervals.

Post Process Step	Agent	Method	Duration	Intervals	Additional Info
Cleaning Step #1	IPA	Ultrasonic	2 min	2	Dry after each interval
Dry	n.a.	Compressed air	10 s to 60 s	1	Air pressure (50psi)
Wait before post curing	n.a.	Ambient condition	60 min	1	Room temperature

POST CURING

LOCTITE 3D MED3394 WH requires post curing to achieve specified properties. It is recommended that either an LED or wide spectrum lamp be used to post cure parts.

An additional heat cure at 100°C for one hour is recommended for most workflows to realize highest HDT performance. Allow the parts to rest one hour between UV cure and heat cure. To minimize risk of warpage place parts in cold oven before ramping up temperature to target value and cool down parts slowly in switched off oven after reaching the heat curing conditions.

UV Curing Unit	UV Source	Intensity	Cure time per side	Additional Settings (Shelf, Output Energy)
Dymax 5000 EC Flood	Mercury Arc Bulb (broad spectrum)	150 mW/cm ² at 380 nm	20 min	400W, Shelf K
Loctite CL36	405nm LED	80 mW/cm ² at 405 nm	20 min	100% top & side



LOCTITE®

MED3394™
STERILIZABLE
WHITE



WORKFLOW

Validated workflows need to be followed to achieve properties as provided in the TDS. Examples of validated workflow steps are listed below. Users should defer to the most current workflow information for best results which can be found at <https://www.loctiteam.com/printer-validation-settings>

STORAGE

Store **LOCTITE 3D MED3394 WH** in the unopened container in a dry location. Optimal Storage: 8°C to 30°C. Storage below 8°C or above 30°C can adversely affect product properties. Material removed from containers may be contaminated during use. For this reason, filter used resin with 190 µm mesh filter before placing back into proper storage container.









MED3394™ STERILIZABLE WHITE



AGEING AND ENVIRONMENTAL EFFECTS – STERILIZATION

LOCTITE 3D MED3394 WH was sterilized via a variety of sterilization methods. Sterilized samples were conditioned for a minimum of 24 hours before mechanical testing. Control samples were stored at a constant 22°C. All samples were printed using a validated workflow. Mechanical testing was conducted according to ASTM D638 at standard lab conditions (22°C).

Data represents mechanical properties shortly after sterilization and are not indicative of long-term shelf-aged performance.

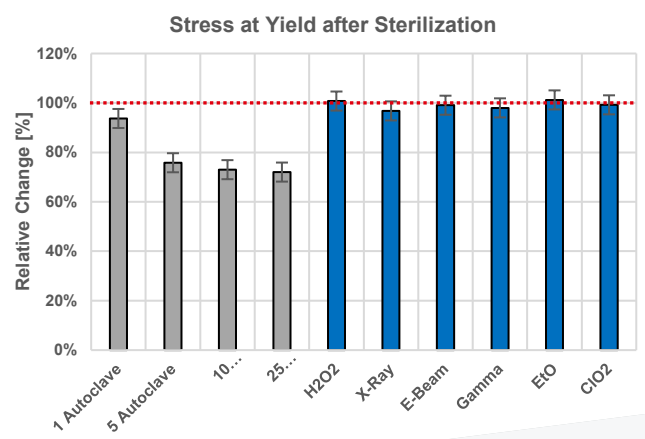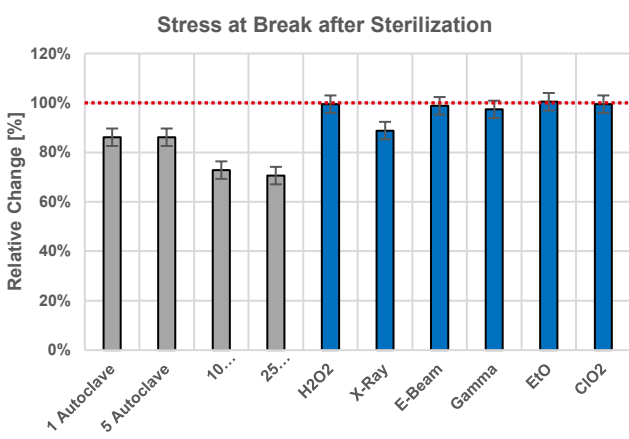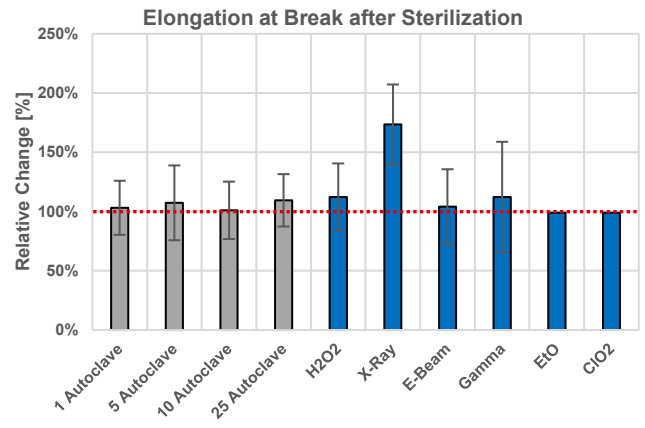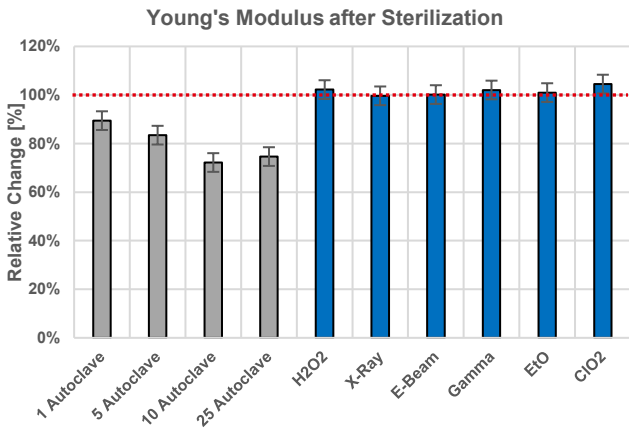

Test parameters:
ASTM D638: Type IV, Pull speed: 5 mm/min, Young's modulus measured at 0.1-1.0% (regression), 22°C. Sterilization Information: Autoclave – 134°C for 18 minutes at 2.1 bar, H2O2 – 4 injection sterilization cycle of 59% H2O2, X-Ray – 11kGy nominal dose, E-Beam – 11kGy nominal dose, Gamma – 40kGy nominal dose, ETO – 3 cycles, ClO2 – under vacuum conditions.

Internal Data Sources:
[GEN685128](#)





MED3394™
STERILIZABLE
SHEER BLACK







AGEING AND ENVIRONMENTAL EFFECTS – HEAT AGEING

LOCTITE 3D MED3394 WH was heat aged without load according to ASTM D3045. Test samples were exposed for a defined time at 50°C and conditioned for 24 hours at 22°C before mechanical testing. Control samples were stored at a constant 22°C. All samples were printed in the same print job using a validated workflow. Mechanical testing was conducted according to ASTM D638 at standard lab conditions (22°C).

“0 weeks” represents non-aged samples stored at 22°C and tested 24 hours after post-processing.

Based on temperature dependence of reaction rates a test time of 6 weeks at 50°C can be interpreted as approximately 12 months at ambient temperature.

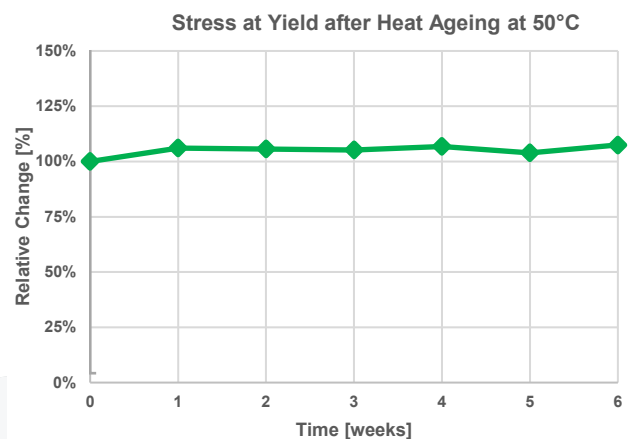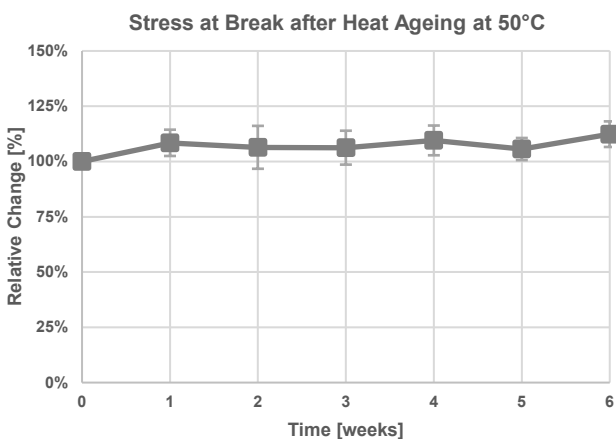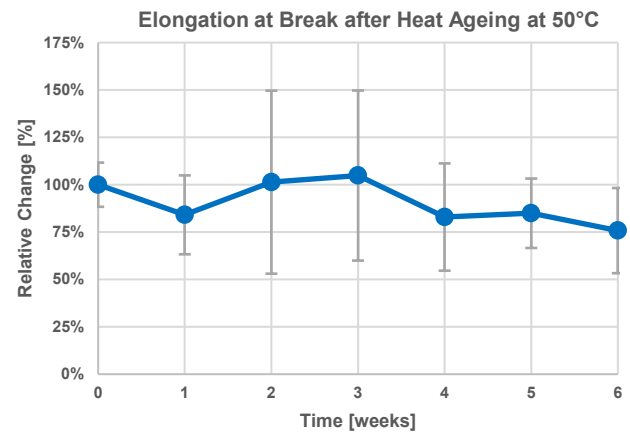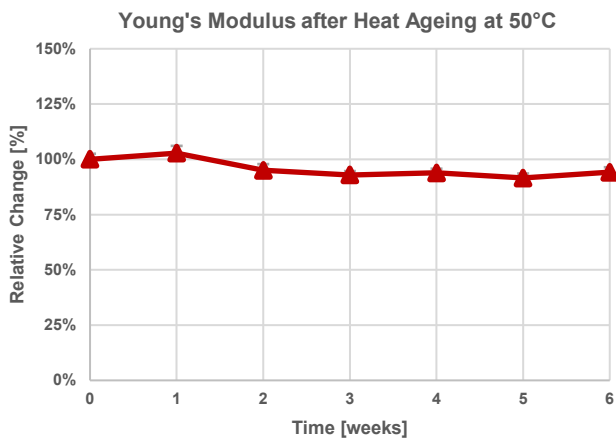

Test parameters:
ASTM D638: Type IV, Pull speed: 5 mm/min, Young's modulus measured at 0.1-1.0% (regression), 22°C

Internal Data Sources:
[FOR704660](#), [FOR704662](#)





MED3394™





STERILIZABLE
SHEER BLACK



AGEING AND ENVIRONMENTAL EFFECTS – ACCELERATED WEATHERING (UV AGEING)

LOCTITE 3D MED3394 WH has been tested after accelerated outdoor weathering according to ASTM D4329 (Cycle A). Test samples were exposed to defined conditions of heat, water condensation and UV light. Exposed samples were conditioned for 24 hours at 22°C before mechanical testing. Control samples were stored at a constant 22°C. All samples were printed in the same print job using a validated workflow. Mechanical testing was conducted according to ASTM D638 at standard lab conditions (22°C). "0 weeks" represents non-aged samples stored at 22°C and tested 24 hours after post-processing.


Please note, accelerated weathering testing can never fully represent real outdoor conditions and complexity. It is therefore recommended to conduct additional (outdoor) testing relevant for your specific application needs.

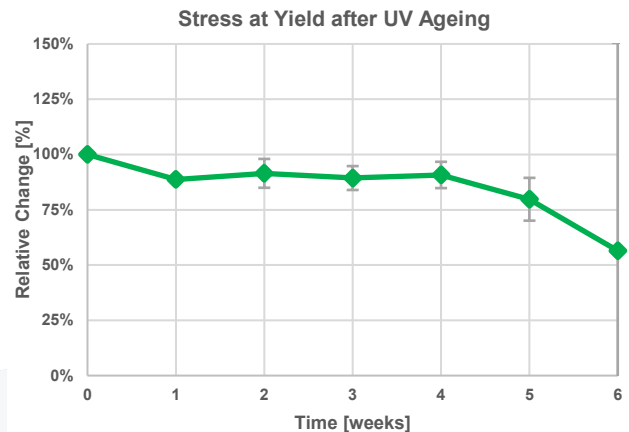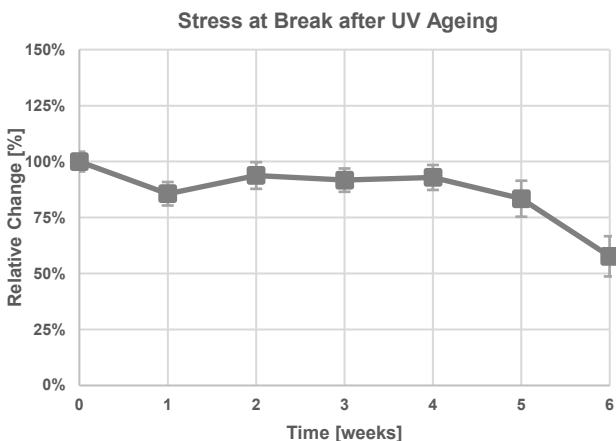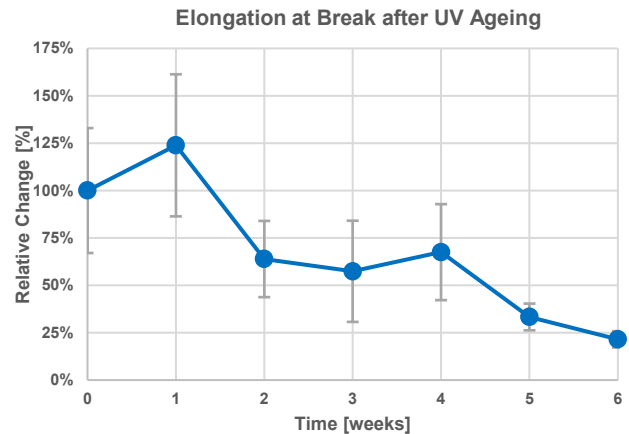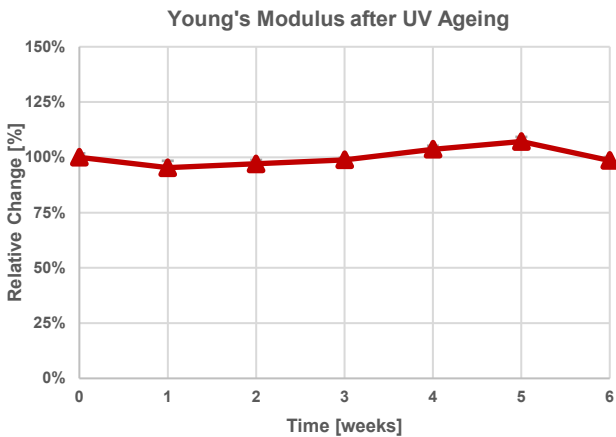

Test parameters:
ASTM D638: Type IV, Pull speed: 5 mm/min, Young's modulus measured at 0.1-1% (regression), 22 °C
ASTM D4329: Cycle A for general applications, QUV/se, UVA 340 nm, 0.89 W/m²·nm, 8 hours UV light at 60°C followed by 4 hours at 50°C condensation in the dark. To reduce any sample warpage during test time samples were placed in tailor-made holders without any fixation clamps or mechanical load. Exposed samples were always removed from QUV before next condensation cycle to avoid samples that are soaked excessively with water before testing.





Internal Data Sources:
[FOR685557](#), [FOR685558](#)



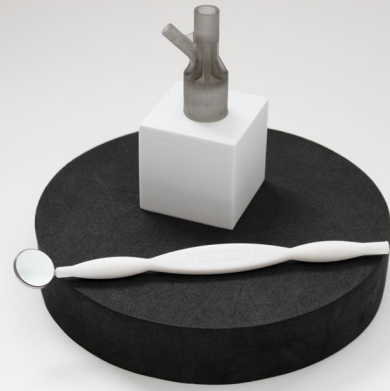

AGEING AND ENVIRONMENTAL EFFECTS – CHEMICAL RESISTANCE MEDICAL

LOCTITE 3D MED3394 WH has been tested after chemical ageing according to ASTM D543. The influence of chemicals was tested by measuring mechanical properties after different test times (Immersion test for 24 and 168 hours). Exposed samples were stored in containers and fully immersed in different chemicals. Samples were stirred every 24 hours using a shaker. After removal, exposed samples were washed and conditioned for 24 hours at 22°C before mechanical testing. All samples were printed using a validated workflow. Mechanical testing was conducted according to ASTM D638 at standard lab conditions (22°C). "100%" represents non-aged samples stored at 22°C and tested 24 hours after post-processing.

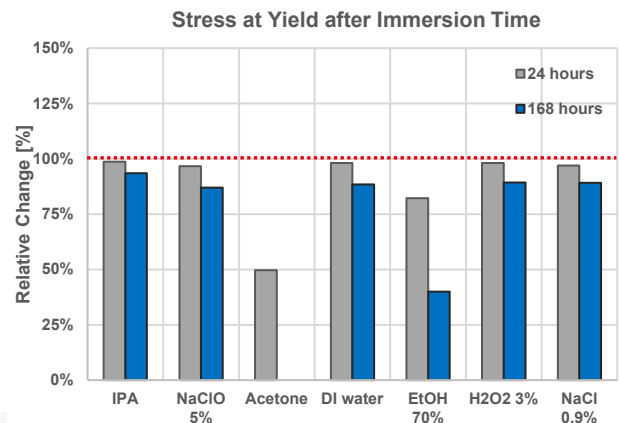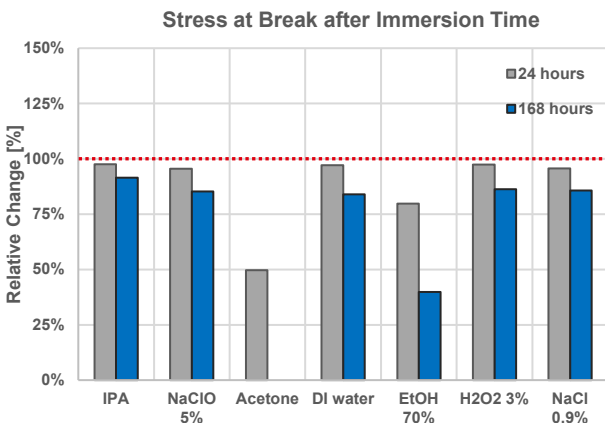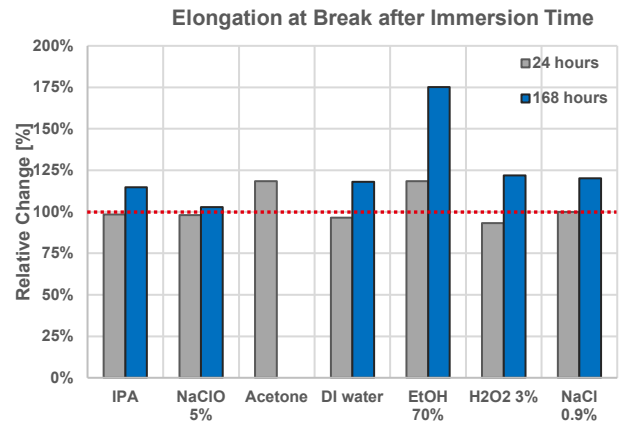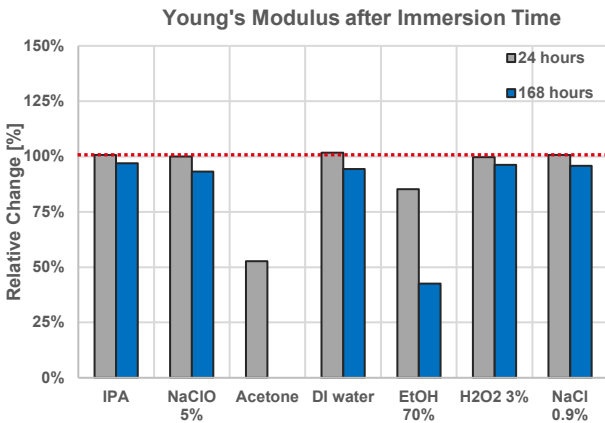

Test parameters:
ASTM D638: Type IV, Pull speed: 5 mm/min, Young's modulus measured at 0.1-1.0% (regression), 22°C
ASTM D543: Samples immersed in different chemicals were stored at 22°C.

Internal Data Sources:
FOR672243, FOR672244, FOR672246, FOR672248, FOR676357, FOR676355, FOR676358






MED3394™
STERILIZABLE
WHITE



AGEING AND ENVIRONMENTAL EFFECTS – CHEMICAL RESISTANCE MASS SOAK

LOCTITE 3D MED3394 SHR BK has been tested after chemical ageing according to ASTM D543. The influence of chemicals was tested by measuring the mass change after different test times (Immersion test for 24 and 168 hours). Exposed samples were stored in containers and fully immersed in different chemicals. Samples were stirred every 24 hours using a shaker. After removal exposed samples were washed, dried and immediately weighed. All samples were printed using a validated workflow.

“100%” represents the initial weight 24 hours after post-processing.

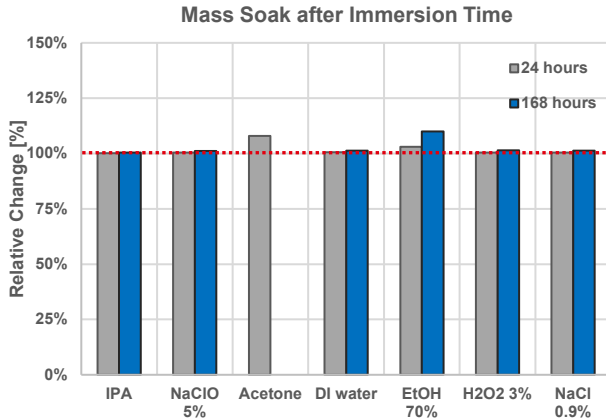

Test parameters:
ASTM D543: Samples immersed in different chemicals were stored at 22°C.

Internal Data Sources:
[FOR672243](#), [FOR672244](#), [FOR672246](#), [FOR672248](#), [FOR676357](#), [FOR676355](#), [FOR676358](#)





MED3394™
STERILIZABLE



NOTE

The information provided in this Technical Data Sheet (TDS) including the recommendations for use and application of the product are based on our knowledge and experience of the product as at the date of this TDS. The product can have a variety of different applications as well as differing application and working conditions in your environment that are beyond our control. Henkel is, therefore, not liable for the suitability of our product for the production processes and conditions in respect of which you use them, as well as the intended applications and results. We strongly recommend that you carry out your own prior trials to confirm such suitability of our product.

Any liability in respect of the information in the Technical Data Sheet or any other written or oral recommendation(s) regarding the concerned product is excluded, except if otherwise explicitly agreed and except in relation to death or personal injury caused by our negligence and any liability under any applicable mandatory product liability law.

In case products are delivered by Henkel Belgium NV, Henkel Electronic Materials NV, Henkel Nederland BV, Henkel Technologies France SAS and Henkel France SA please additionally note the following:

In case Henkel would be nevertheless held liable, on whatever legal ground, Henkel's liability will in no event exceed the amount of the concerned delivery.

In case products are delivered by Henkel Colombiana, S.A.S. the following disclaimer is applicable:

The information provided in this Technical Data Sheet (TDS) including the recommendations for use and application of the product are based on our knowledge and experience of the product as at the date of this TDS. Henkel is not liable for the suitability of our product for the production processes and conditions in respect of which you use them, as well as the intended applications and results. We strongly recommend that you carry out your own prior trials to confirm such suitability of our product.

Any liability in respect of the information in the Technical Data Sheet or any other written or oral recommendation(s) regarding the concerned product is excluded, except if otherwise explicitly agreed and except in relation to death or personal injury caused by our negligence and any liability under any applicable mandatory product liability law.

In case products are delivered by Henkel Corporation, Resin Technology Group, Inc., or Henkel Canada, Inc. the following disclaimer is applicable:

The data contained herein are furnished for information only and are believed to be reliable. We cannot assume responsibility for the results obtained by others over whose methods we have no control. It is the user's responsibility to determine suitability for the user's purpose of any production methods mentioned herein and to adopt such precautions as may be advisable for the protection of property and of persons against any hazards that may be involved in the handling and use thereof. In light of the foregoing, Henkel Corporation specifically disclaims all warranties expressed or implied, including warranties of merchantability or fitness for a particular purpose, arising from sale or use of **Henkel Corporation's products. Henkel Corporation specifically disclaims any liability for consequential or incidental damages of any kind, including lost profits.** The discussion herein of various processes or compositions is not to be interpreted as representation that they are free from domination of patents owned by others or as a license under any Henkel Corporation patents that may cover such processes or compositions. We recommend that each prospective user test his proposed application before repetitive use, using this data as a guide. This product may be covered by one or more United States or foreign patents or patent applications.

Trademark Usage

Except as otherwise noted, all trademarks in this document are trademarks of Henkel Corporation in the U.S. and elsewhere. ® denotes a trademark registered in the U.S. Patent and Trademark Office.



LOCTITE®



FIND OUT MORE AT
LOCTITEAM.COM

LOCTITE®
Henkel Corporation
loctite3dp@henkel.com

